

## Method And Apparatus To Optimally Measure Cardiac Depolarization/Repolarization Instability Inventor: David W. Mortara Attorney Docket No. 2395-00033

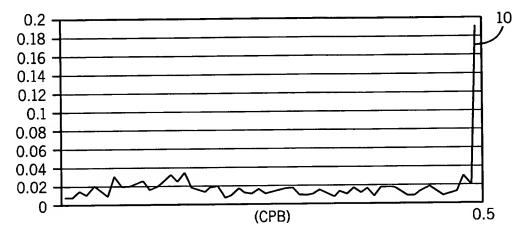


FIG. 2a




FIG. 2b

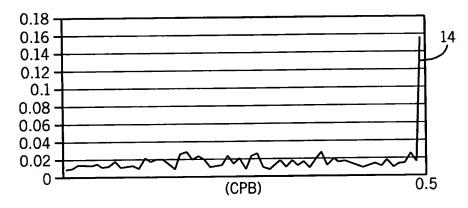


FIG. 2c

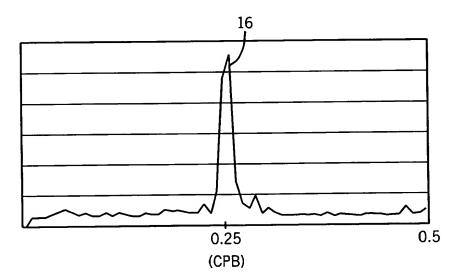


FIG. 3a

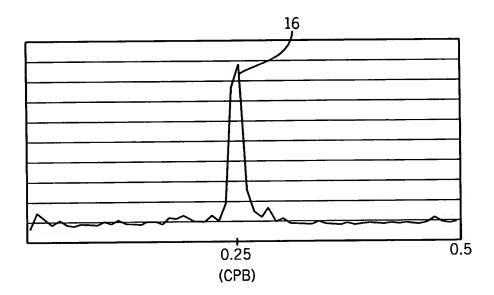


FIG. 3b

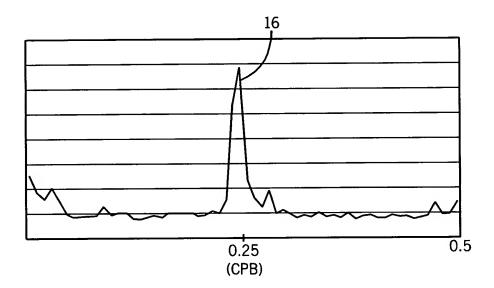


FIG. 3c

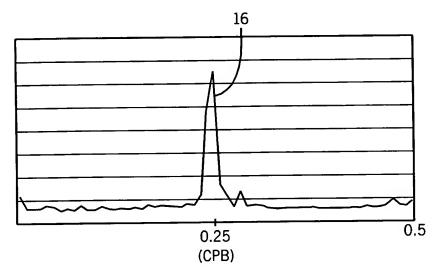


FIG. 3d

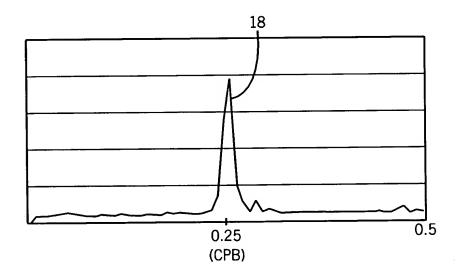


FIG. 3e

Method And Apparatus To Optimally Measure Cardiac Depolarization/Repolarization Instability Inventor: David W. Mortara Attorney Docket No. 2395-00033


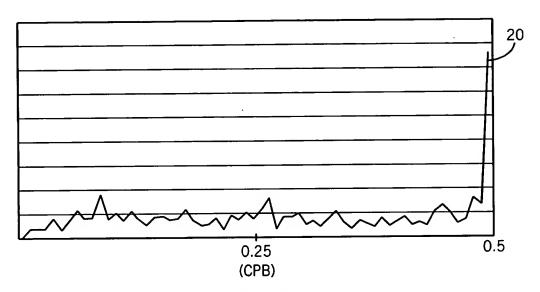


FIG. 3f

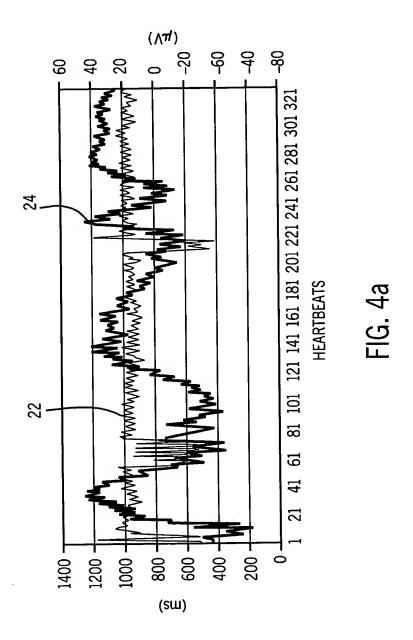

Method And Apparatus To Optimally Measure Cardiac Depolarization/Repolarization Instability Inventor: David W. Mortara Attorney Docket No. 2395-00033

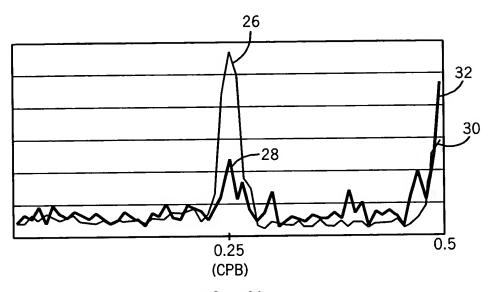


FIG. 4b